10/549409

App No.: Not Yet Assigned Docket No.: HO-P03225US0 Inventor: Roque H. Ferreyro, Irigoyen et al.
Title: HYDRAULIC DEVICE FOR THE INJECTION OF BONE CEMENT IN PERCUTANEOUS VERTEBROPLASTY Fulbright & Jaworski L.L.P./713-651-5407

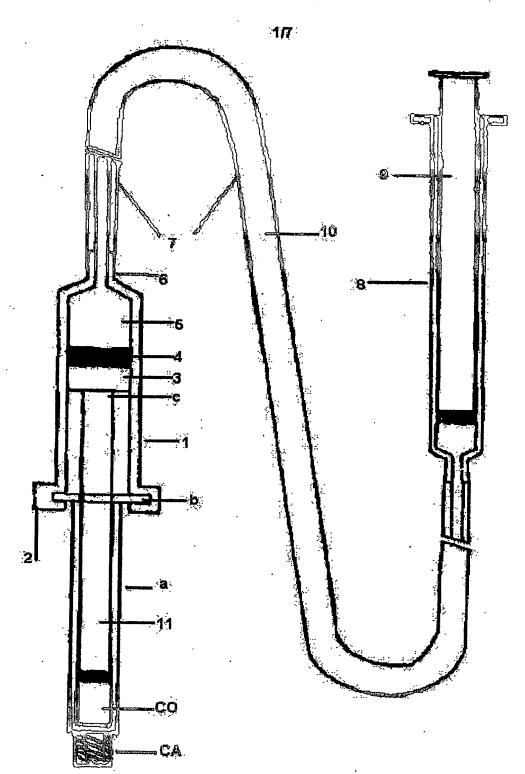



Fig./

App No.: Not Yet Assigned Docket No.: HO-P03225US0 Inventor: Roque H. Ferreyro, Irigoyen et al.
Title: HYDRAULIC DEVICE FOR THE INJECTION OF BONE CEMENT IN PERCUTANEOUS VERTEBROPLASTY Fulbright & Jaworski L.L.P./713-651-5407




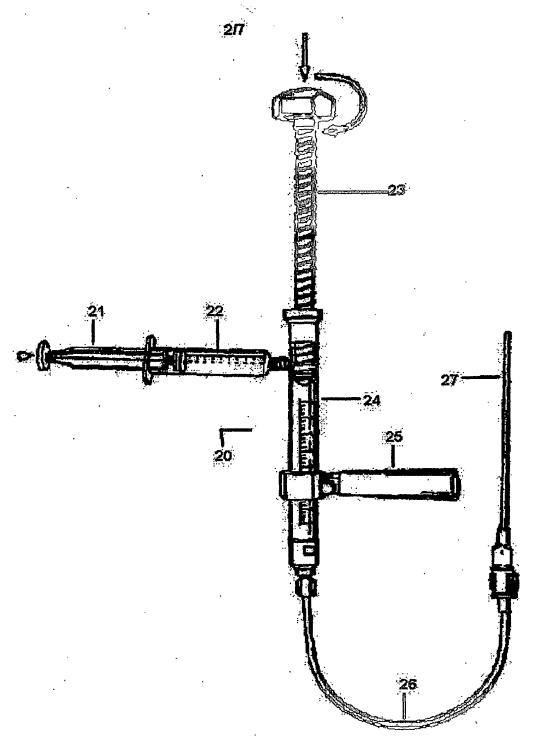


Fig. 2

App No.: Not Yet Assigned Docket No.: HO-P03225US0 Inventor: Roque H. Ferreyro, Irigoyen et al.
Title: HYDRAULIC DEVICE FOR THE INJECTION OF BONE CEMENT IN PERCUTANEOUS VERTEBROPLASTY Fulbright & Jaworski L.L.P./713-651-5407



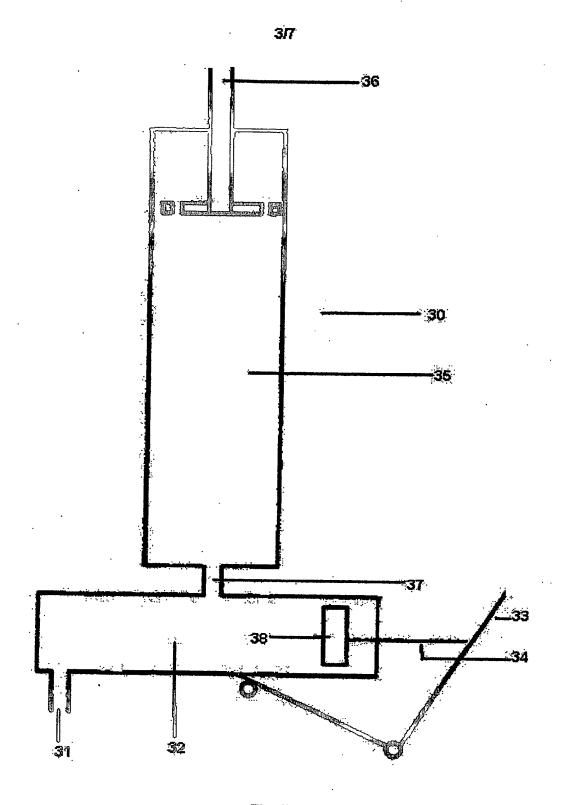

Flg. 3

App No.: Not Yet Assigned Docket No.: HO-P03225US0 Inventor: Roque H. Ferreyro, Irigoyen et al.

Title: HYDRAULIC DEVICE FOR THE INJECTION OF BONE CEMENT IN PERCUTANEOUS VERTEBROPLASTY

Fulbright & Jaworski L.L.P./713-651-5407

10/549409

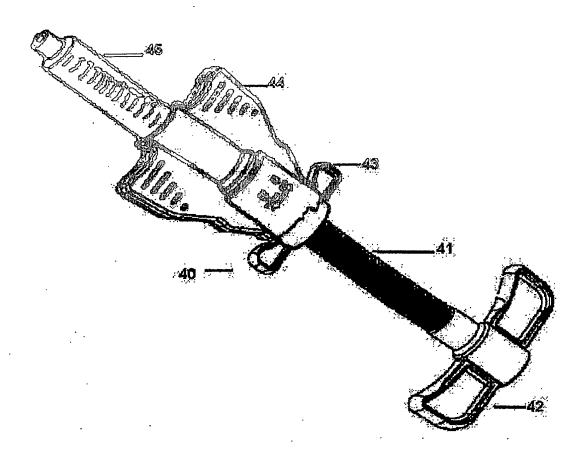


Fig. 4

App No.: Not Yet Assigned Docket No.: HO-P03225US0 Inventor: Roque H. Ferreyro, Irigoyen et al. Title: HYDRAULIC DEVICE FOR THE INJECTION OF BONE

CEMENT IN PERCUTANEOUS VERTEBROPLASTY

Fulbright & Jaworski L.L.P./713-651-5407

10/549409



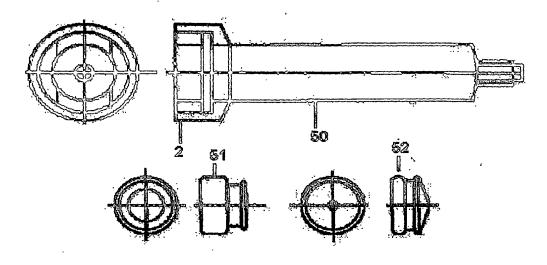


Fig. 5

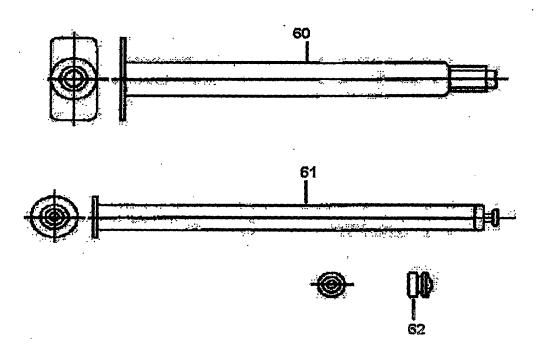



Fig. 6

App No.: Not Yet Assigned Docket No.: HO-P03225US0 Inventor: Roque H. Ferreyro, Irigoyen et al. Title: HYDRAULIC DEVICE FOR THE INJECTION OF BONE CEMENT IN PERCUTANEOUS VERTEBROPLASTY Fulbright & Jaworski L.L.P./713-651-5407





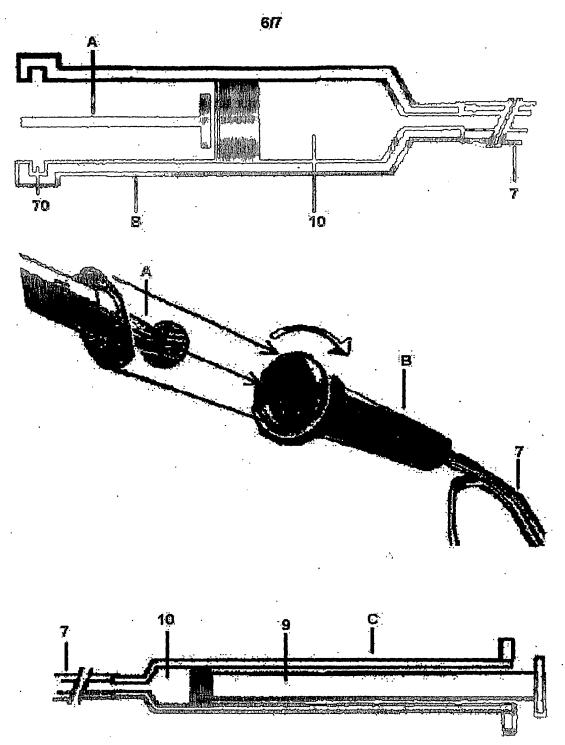


Fig. 7

App No.: Not Yet Assigned Docket No.: HO-P03225US0 Inventor: Roque H. Ferreyro, Irigoyen et al. Title: HYDRAULIC DEVICE FOR THE INJECTION OF BONE CEMENT IN PERCUTANEOUS VERTEBROPLASTY Fulbright & Jaworski L.L.P./713-651-5407



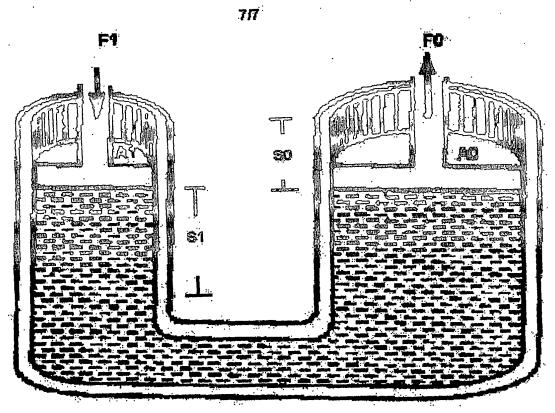

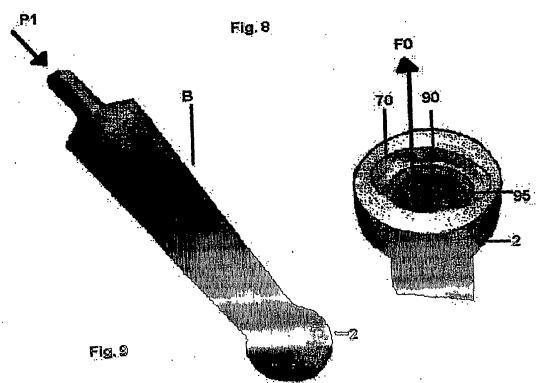

This Page is Inserted by IFW Indexing and Scanning Operations and is not part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:
☐ BLACK BORDERS
☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES
FADED TEXT OR DRAWING
☐ BLURRED OR ILLEGIBLE TEXT OR DRAWING
☐ SKEWED/SLANTED IMAGES
☐ COLOR OR BLACK AND WHITE PHOTOGRAPHS
☐ GRAY SCALE DOCUMENTS
☐ LINES OR MARKS ON ORIGINAL DOCUMENT
☐ REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY
Потивъ

IMAGES ARE BEST AVAILABLE COPY.

As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.